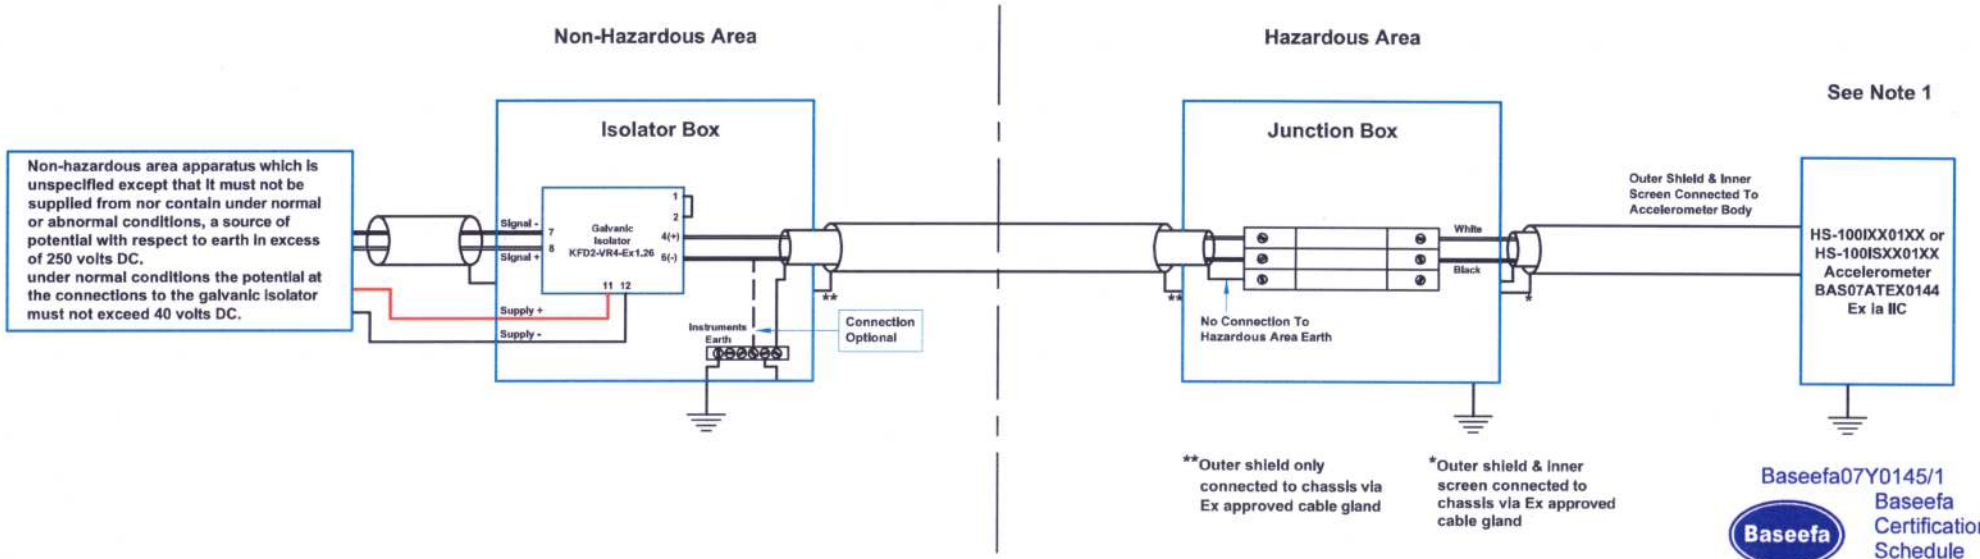

Baseefa07Y0145/1
Baseefa Certification Schedule Drawing

D.S. Kerfoot

Table 1: Cable Parameters For Additional Cable Lengths

Group	Capacitance µF	L/R Ratio µH/Ω
Accelerometer With Integral Cable Length ≤ 10m		
IIC	0.086	46
IIB	0.730	172
IIA	2.470	363
Accelerometer With Integral Cable Length ≤ 50m		
IIC	0.051	46
IIB	0.695	172
IIA	2.435	363
Accelerometer With Integral Cable Length ≤ 92m		
IIC	0.013	46
IIB	0.657	172
IIA	2.397	363

Hansford Sensors Ltd

HS-100I or HS-100IS
Accelerometer System
Baseefa07Y0145/1
Ex ia IIC T4 (-55°C ≤ Ta ≤ +110°C) or
Ex ia IIC T6 (-55°C ≤ Ta ≤ +60°C)

Notes:

1. The capacitance and inductance, to resistance ratio (L/R) of hazadous area cable, must not exceed the values shown in Table 1.

2. The installer is to perform a risk assesment in accordance with clause 10 of EN 60079-25 and install lightning protection arrestors as deemed necessary.

Rev No	DRF No	Date Drg	Drg By	Appd By
A	Release	15/06/07	MJS	CMH
B	DFR0164	13/01/11	MJS	CMH

Material: N/A

Tolerances Unless Stated
0 or 0.0 ±0.5
0.00 ±0.15
Angle ±5°
1.6 Finish All Over
Threads g6 H6

Hansford Sensors
Excellence in Vibration Monitoring
Hansford Sensors Ltd
Artisan, Hillbottom Rd
Sands Industrial Estate
High Wycombe
Bucks HP12 4HJ

Do Not Scale

All Dimensions In mm Unless Otherwise Stated

If In Doubt - Ask!

Description: System Connections For HS-100I & HS-100IS Group II Accelerometers With Armoured Cable F.U.W. Galvanic Isolation

Drawing No: M06-003-B

Scale: NTS

Sheet: 1 of 2

Form Number: QF024 Issue 1